



Certificate of Analysis


| | | | |
|------------------|-------------------------------|----------------------|---------------------------|
| Date: | 2025-07-01 11:50:44 -04:00 | Cultivar: | |
| Serial: | LL030645 | Moisture: | 0.0% |
| LightLab | BW-LABS | Col Tests Remaining: | 6 |
| Operator: | DAIANA | CoA Revision: | 0 |
| Sample ID: | | Calibration Exp: | 2026-03-21 |
| Method: | LightLab HPLC | Product: | Canna Drops 175 mg D9 THC |
| Test Type: | Nanoemulsion Liquid (%weight) | SKU: | |
| Weight / Volume: | 0.455 g | Batch: | SECD3174 |
| Solvent: | 20 ml | | |
| Temperature: | 25.3 °C | | |
| Notes: | | | |

Cannabinoid Profile

| Analyte | Per 60.000 g Serving (mg) | Per 1.0 Pieces(mg) | % | LOQ |
|---------------------------|---------------------------|--------------------|-------------|--------|
| THC-A | ND | ND | ND | 0.0071 |
| Δ9-THC | 182.1 | 182.1 | 0.30 | 0.0071 |
| CBD-A | ND | ND | ND | 0.0071 |
| CBG-A | ND | ND | ND | 0.0071 |
| CBD/CBG | ND | ND | ND | 0.0071 |
| CBN-A | ND | ND | ND | 0.0071 |
| CBN | ND | ND | ND | 0.0071 |
| CBC-A | ND | ND | ND | 0.0071 |
| CBC | ND | ND | ND | 0.0071 |
| Δ8-THC* | ND | ND | ND | 0.057 |
| Δ10-THC | ND | ND | ND | 0.0071 |
| THCV-A | ND | ND | ND | 0.0071 |
| THCV | ND | ND | ND | 0.0071 |
| Terpenes | | | Low | |
| Total THC | 182.1 | 182.1 | 0.30 | |
| Total Cannabinoids | 182.1 | 182.1 | 0.30 | |

ND = Not Detected; n/a = Not Analyzed; LOQ = Limit of Quantification; Total THC = $(0.877 \times \text{THC-A}) + \Delta 9\text{-THC}$; Total CBD = $(0.877 \times \text{CBD-A}) + \text{CBD}$. * Δ8THC has lower precision and higher detection limit than other cannabinoids.

Chromatogram

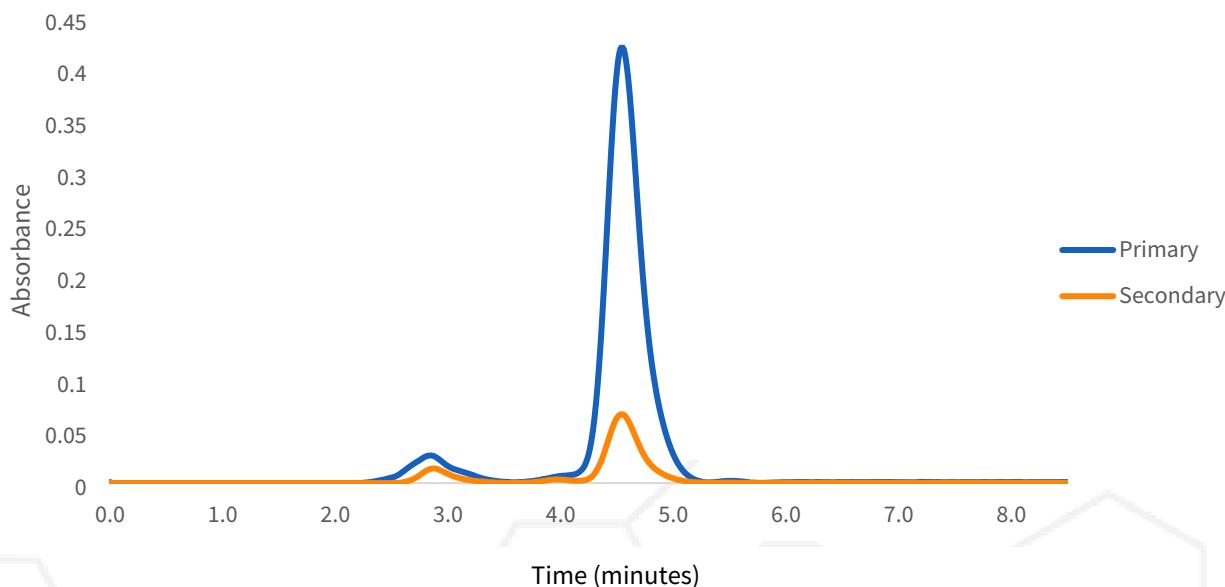

Sample Images



Change History

| Date | User | Action |
|----------------------------|------|--|
| 2025-07-01 11:50:44 -04:00 | | Test Recorded |
| 2025-07-01 12:10:43 -04:00 | DA | Added an image |
| 2025-07-01 12:11:46 -04:00 | DA | Changed Operator from "" to "DAIANA". Changed EdblProduct from "" to "Canna Drops 175 mg D9 THC". Changed Batch from "" to "SECD3174". |
| 2025-07-01 12:12:02 -04:00 | | Generated a CoA (revision 0) |



7/1/2025



Scan for Authenticity

Approved

Date

The signatory confirms that the Operator has performed the sample preparation according to the LightLab User's Guide. This report is for quality assurance purposes only. These results relate only to the sample included on this report. Orange Photonics makes no claims as to the efficacy, safety, or risks associated with any detected or non-detected level of any compounds reported herein. Orange Photonics makes no claims regarding the adherence to sample preparation guidelines, by the operator, as outlined in the LightLab User's Guide.

